

PRODUCT CONFORMITY CERTIFICATE

This is to certify that the

AR602Z/Hg

Manufactured by:

Opsis AB
P.O. Box 244
S-244 02 Furulund
Sweden


has been assessed by CSA Group
and for the conditions stated on this certificate complies with:

Environment Agency Guidance
“MCERTS for stack emissions monitoring equipment at industrial installations”
- Continuous emissions monitoring systems (CEMS)
Published 20 October 2020
EN 15267-1:2009, EN15267-2:2009, EN 15267-3:2007
& QAL 1 as defined in EN 14181: 2014

Certification ranges:

Hg 0 to 45 µg/m³
 0 to 100 µg/m³

Project number: 80137645
Certificate number: Sira MC120201/02
Initial certification: 25 September 2012
This certificate issued: 16 September 2022
Renewal date: 24 September 2027



Andrew Young
Environmental Team Manager

MCERTS is operated on behalf of the Environment Agency by

CSA Group Testing UK Ltd

Unit 6, Hawarden Industrial Park
Hawarden, Deeside, CH5 3US
Tel: +44 (0)1244 670 900



0011

*The MCERTS certificate consists of this document in its entirety.
For conditions of use, please consider all the information within.
This certificate may only be reproduced in its entirety and without change
To authenticate the validity of this certificate please visit www.csagroupuk.org/mcerts*

Certificate Contents

Approved Site Application.....	2
Basis of Certification	2
Product Certified.....	3
Certified Performance	4
Description.....	7
General Notes	7

Approved Site Application

Any potential user should ensure, in consultation with the manufacturer, that the monitoring system is suitable for the intended application. For general guidance on monitoring techniques refer to the Environment Agency Monitoring Technical Guidance Notes available at www.mcerts.net

This instrument is considered suitable for use on waste incineration and large combustion plants. This CEMS has been proven suitable for its measuring task (parameter and composition of the flue gas) by use of the QAL 1 procedure specified in EN14181. The lowest certified range for each determinand shall not be more than 1.5 times the daily average emission limit value (ELV) for incineration plants, and not more than 2.5 times the ELV for other types of applications.

Basis of Certification

This certification is based on the following test report(s) and on CSA Group's assessment and ongoing surveillance of the product and the manufacturing process:

TÜV Rheinland Report Number 936/21215492/A dated 10 October 2011


The field test was conducted on a municipal waste incinerator from 6 May 2011 to 23 August 2011.

Certificate No: Sira MC120201/02
This Certificate issued: 16 September 2022

*This certificate may only be reproduced in its entirety and without change
To authenticate the validity of this certificate please visit www.csagroupuk.org/mcerts*

Product Certified

The AR602Z/Hg measuring system consists of the following parts:

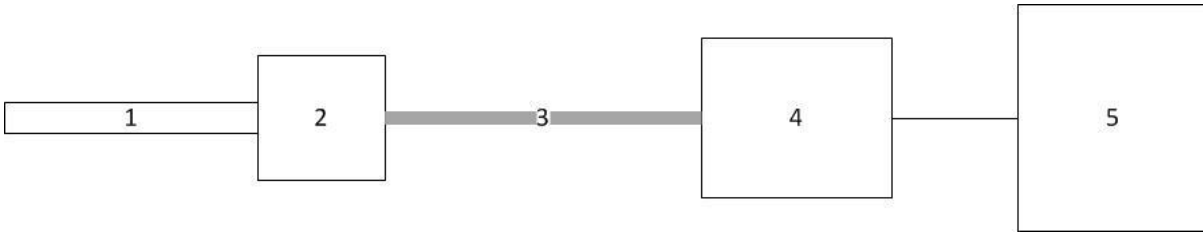

1. Sample Probe	2. Heated Filter	3. Heated Sample Line	4. Gas Conditioning	5. Analyser
Model: Opsis HF100	Model: Opsis HF100	Model: Opsis HL100 10m	Model: Opsis HC100	Model: AR602 UV analyser

This certificate applies to all instruments fitted with software version 7.21 (serial number 1498 onwards).

Certificate No: Sira MC120201/02
 This Certificate issued: 16 September 2022

*This certificate may only be reproduced in its entirety and without change
 To authenticate the validity of this certificate please visit www.csagroupuk.org/mcerts*

Certified Performance

The instrument was evaluated for use under the following conditions:

Ambient Temperature Range: 5°C to 40°C
 Instrument IP rating: IP20: Analyser*, must be placed in a protected area
 IP54: Duct mounted parts (transmitter & receiver unit)

*Must be installed in an environment which protects it from dust and splash water (closed measuring rack)

Results expressed are for range 0 to 45 µg/m³ unless otherwise stated.

Test	Results expressed as % of the certification range				Other results	MCERTS specification
	<0.5	<1	<2	<5		
Response time						
Hg					140s	<200s
Hg (0 to 100mg/m ³)					140s	<200s
Repeatability standard deviation at zero point						
Hg	0.40					<2.0%
Repeatability standard deviation at reference point						
Hg	0.40					<2.0%
Lack-of-fit						
Hg			1.56			<2.0%
Hg (0 to 100mg/m ³)			-1.40			<2.0%
Influence of ambient temperature zero point						
Hg	-0.40					<5.0%
Influence of ambient temperature reference point						
Hg		0.70				<5.0%
Influence of sample gas flow for extractive CEMS						
Hg	-0.20					<2.0%
Influence of voltage variations 320 to 420V						
All gases		-0.90				<2.0%

Certificate No: Sira MC120201/02
 This Certificate issued: 16 September 2022

*This certificate may only be reproduced in its entirety and without change
 To authenticate the validity of this certificate please visit www.csagroupuk.org/mcerts*

Test	Results expressed as % of the certification range				Other results	MCERTS specification
	<0.5	<1	<2	<5		
Cross-sensitivity at zero with interferents: O ₂ , H ₂ O, CO, CO ₂ , CH ₄ , N ₂ O, NO, NO ₂ , NH ₃ , SO ₂ , HCl Hg			-1.55		Note 2	<4.0%
Cross-sensitivity at reference with interferents: O ₂ , H ₂ O, CO, CO ₂ , CH ₄ , N ₂ O, NO, NO ₂ , NH ₃ , SO ₂ , HCl Hg				2.67	Note 2	<4.0%
Measurement uncertainty Hg					Guidance - at least 25% below max permissible uncertainty 9.3%	
Calibration function (field) Hg					>0.9891	>0.90
Response time (field) Hg					288 Note 1 Note 3	<200s
Lack of fit (field) Hg			1.89			<2.0%
Maintenance interval					4 weeks Note 4	>8 days

Certificate No: Sira MC120201/02
 This Certificate issued: 16 September 2022

*This certificate may only be reproduced in its entirety and without change
 To authenticate the validity of this certificate please visit www.csagroupuk.org/mcerts*

Test	Results expressed as % of the certification range				Other results	MCERTS specification
	<0.5	<1	<2	<5		
Zero and Span drift requirement	<p>In order to determine zero and span drift, zero and sample gas have to be admitted with the help of an external test gas generator at regular intervals (at least once per maintenance interval). The measuring system does not have a mechanism to compensate for zero and span drift.</p> <p>The received light level is analysed and displayed for each measurement. If the light level falls below a specified level (e.g. due to contamination), a status signal is set.</p>					<p>Clause 6.13 & 10.13</p> <p>Manufacturer shall provide a description of the technique to determine and compensate for zero and span drift.</p>
Change in zero point over maintenance interval Hg				1.7		<3.0%
Change in reference point over maintenance interval Hg				-2.5		<3.0%
Availability					98.4%	>95%
Reproducibility Hg			1.6			<3.3%

Note 1: The response time reported in the field test does not meet the requirement for EN15267-3. However, this extended time was caused by a significant lag time caused by the volume of the test rig.

Note 2: In order to compensate for cross-sensitivity, the SO₂ content has to be determined in the measuring cell.

Note 3: During the laboratory and field test a heated test gas line of 10m length was used.

Note 4: The AR602Z/Hg has a maintenance interval of four weeks. The work detailed below has to be carried out at regular intervals, depending on local conditions:

Monthly maintenance activities:

- Visual inspection of the entire AMS,
- Checking of target temperatures of the probe, heated line, converter and measuring cell,
- Checking of the measured light level,
- Checking of the zero point by admitting wet synthetic air to the test gas connection of the probe,
- Checking of the reference point by admitting Hg sample gas obtained from an evaporated HgCl₂ solution to the test gas connection of the probe. Checking of the reference point requires a test gas generator (e.g. Type HovaCal) as well as a suitable HgCl₂-solution.

Biannual maintenance activities:

Replacement of the xenon lamps

The test lab suggests to schedule several days for necessary adjustment and maintenance works in order to avoid outing times, which exceed the limits stipulated in the 13th and 17th BImSchV.

Certificate No: Sira MC120201/02
This Certificate issued: 16 September 2022

*This certificate may only be reproduced in its entirety and without change
To authenticate the validity of this certificate please visit www.csagroupuk.org/mcerts*

Description

The measurement of mercury atoms is made with UV DOAS. Mercury molecules such as HgCl₂ are converted into atomic mercury in a catalytic converter. The system is hot wet extractive system using a probe, filter, converter, measurement cell and ejector pump where all components are heated. The AR602 UV DOAS analyzer used in the mercury system can measure other components such as SO₂, NO_x and NH₃.

General Notes

1. This certificate is based upon the equipment tested. The Manufacturer is responsible for ensuring that on-going production complies with the standard(s) and performance criteria defined in this certificate. The manufacturer is required to maintain an approved quality management system controlling the manufacture of the certified product. Both the product and the quality management system shall be subject to regular surveillance according to 'Regulations Applicable to the Holders of CSA Group Testing UK Ltd Certificates'.
2. The design of the product certified is held and maintained by TÜV Rheinland for certificate No. Sira MC120201.
3. If a certified product is found not to comply, CSA Group should be notified immediately at the address shown on this certificate.
4. The certification marks that can be applied to the product or used in publicity material are defined in 'Regulations Applicable to the Holders of CSA Group Testing UK Ltd Certificates'.
5. This document remains the property of CSA Group and shall be returned when requested by CSA Group.

Certificate No: Sira MC120201/02
This Certificate issued: 16 September 2022

*This certificate may only be reproduced in its entirety and without change
To authenticate the validity of this certificate please visit www.csagroupuk.org/mcerts*